CERTIFICATE OF ANALYSIS

Product Polymethyl methacrylate **Mp 1,591,000**

Batch Number 0006577329

Part Numbers PL2024-2001, PL2024-2005, PL2024-2010

	GPC	Light scattering	Viscometry
Mp (g/mol)	1,591,000		
Mn (g/mol)	1,439,000		
Mw (g/mol)	1,531,000	1,477,000	
Mv (g/mol)	1,519,000		
	Mw/Mn = 1.06		[η] = 2.0732 dl/g

Mp, Mn, Mw & Mv are the respective peak, number, weight and viscosity molecular weight averages

Mw/Mn = molecular weight distribution or polydispersity ratio [η] = Intrinsic viscosity

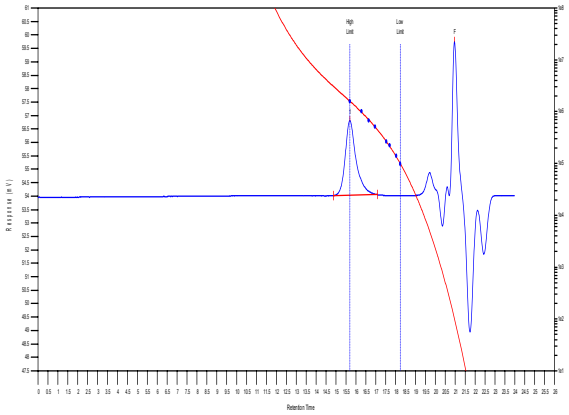

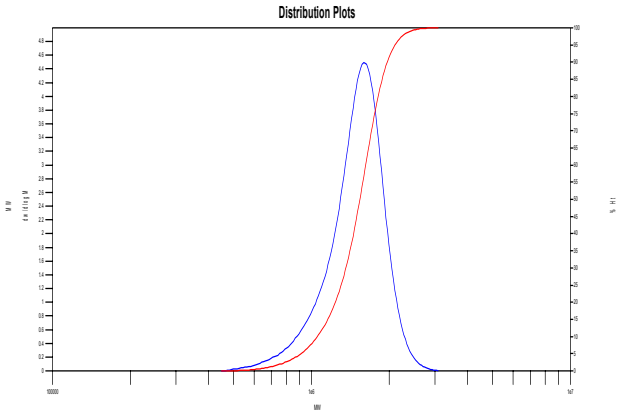

Analysis Conditions

	GPC	Light scattering	Viscometry
System	Cirrus GPC / SEC	Agilent 1260 GPC/SEC MDS	Agilent 1260 GPC/SEC MDS
Detector	Refractive index	1260 Infinity Dual Angle LS	1260 Infinity Viscometer
Columns	2 x PLgel 10e6Å 10µm 300x7.5mm	PLgel 10µm MIXED-BLS 300x7.5mm	PLgel 10µm MIXED-BLS 300x7.5mm
Solvent	THF	THF	THF
Flow rate	1.0 ml / min	1.0 ml / min	1.0 ml / min
Injection volume	20µl	100µl	100µl
Sample concentration	0.05%	0.67640 mg / ml	0.67640 mg / ml
Temperature	Ambient	30°C	30°C
Calibrants	Polymethylmethacrylate	Polystyrene	Polystyrene
Angle		15°	
dn/dc		0.085 g/ml	

The above characterisation data has been measured according to our Quality Control procedures.

Certificate of Analysis valid until expiry date – 2nd January 2031

Agilent Manufacturing Site: Essex Road, Church Stretton, Shropshire, SY6 6AX, UK

G.K.Harmer P.C.Link

Quality Department

Issue 1 19th January 2021 COA STANDARDS 1 Rev 1.04