CERTIFICATE OF ANALYSIS

Product Polystyrene **Mp 1,069,000**

Batch Number 0006575348

Part Numbers PL2014-1001, PL2014-1005, PL2014-1010

	GPC	Light scattering	Viscometry
Mp (g/mol)	1,069,000		
Mn (g/mol)	1,016,000		
Mw (g/mol)	1,056,000	1,001,000	
Mv (g/mol)	1,051,000		
	Mw/Mn = 1.04		[η] = 2.2877 dl/g

Mp, Mn, Mw & Mv are the respective peak, number, weight and viscosity molecular weight averages

Mw/Mn = molecular weight distribution or polydispersity ratio [η] = Intrinsic viscosity

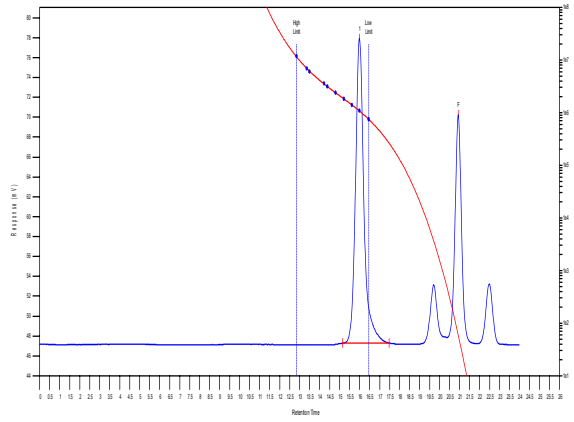

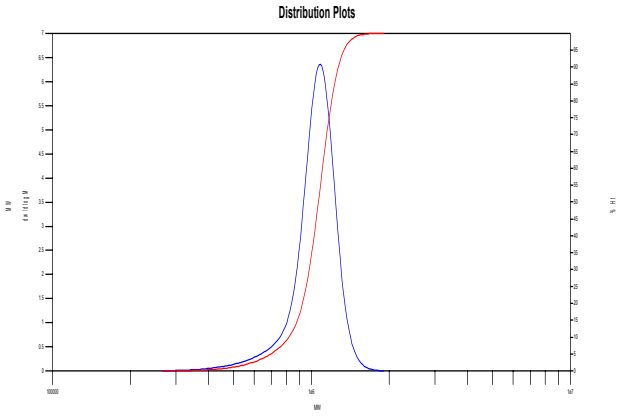

Analysis Conditions

	GPC	Light scattering	Viscometry
System	Cirrus GPC / SEC	Agilent 1260 GPC/SEC MDS	Agilent 1260 GPC/SEC MDS
Detector	Ultra violet	1260 Infinity Dual Angle LS	1260 Infinity Viscometer
Columns	2 x PLgel 106Å 10µm 300x7.5mm	PLgel 10µm MIXED-BLS 300x7.5mm	PLgel 10µm MIXED-BLS 300x7.5mm
Solvent	THF	THF	THF
Flow rate	1.0 ml / min	1.0 ml / min	1.0 ml / min
Injection volume	20µl	100µl	100µl
Sample concentration	0.01%	0.29800 mg / ml	0.29800 mg / ml
Temperature	Ambient	30°C	30°C
Calibrants	Polystyrene	Polystyrene	Polystyrene
Angle		15°	
dn/dc		0.185 g/ml	

The above characterisation data has been measured according to our Quality Control procedures.

Certificate of Analysis valid until expiry date – 2nd January 2031

Agilent Manufacturing Site: Essex Road, Church Stretton, Shropshire, SY6 6AX, UK

M.Griffin P.C.Link

Quality Department

Issue 1 15th January 2021 COA STANDARDS 1 Rev 1.04