CERTIFICATE OF ANALYSIS

Product Polystyrene **Mp 6430**

Batch Number 0006582217

Part Numbers PL2012-8001, PL2012-8005, PL2012-8010

	GPC	Light scattering	Viscometry
Mp (g/mol)	6430		
Mn (g/mol)	6200		
Mw (g/mol)	6370	7070	
Mv (g/mol)	6340		
	Mw/Mn = 1.03		[η] = 0.0699 dl/g

Mp, Mn, Mw & Mv are the respective peak, number, weight and viscosity molecular weight averages
Mw/Mn = molecular weight distribution or polydispersity ratio [η] = Intrinsic viscosity

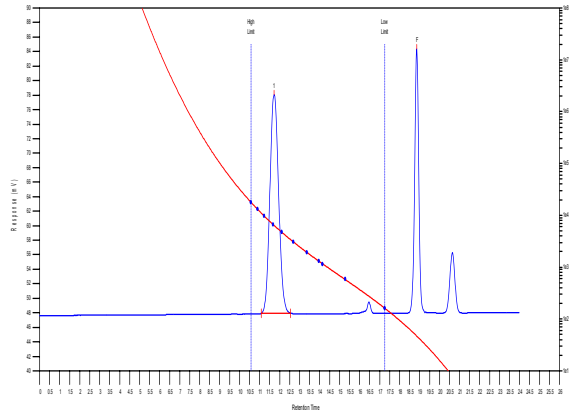

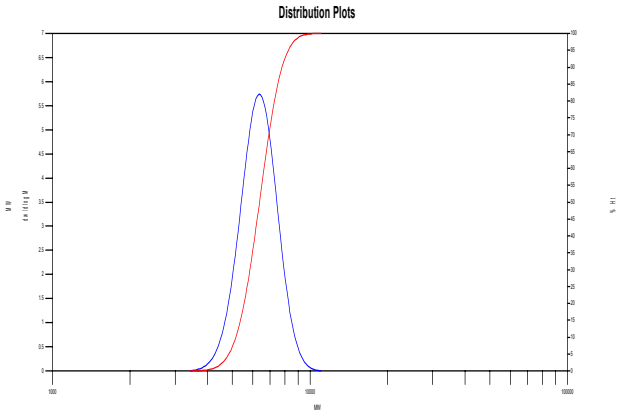

Analysis Conditions

	GPC	Light scattering	Viscometry
System	Cirrus GPC / SEC	Agilent 1260 GPC/SEC MDS	Agilent 1260 GPC/SEC MDS
Detector	Ultra violet	1260 Infinity Dual Angle LS	1260 Infinity Viscometer
Columns	2 x PLgel 5µm 500Å 300x7.5mm	PLgel 10µm MIXED-BLS 300x7.5mm	PLgel 10µm MIXED-BLS 300x7.5mm
Solvent	THF	THF	THF
Flow rate	1.0 ml / min	1.0 ml / min	1.0 ml / min
Injection volume	20µl	100µl	100µl
Sample concentration	0.05%	8.04720 mg / ml	8.04720 mg / ml
Temperature	Ambient	30°C	30°C
Calibrants	Polystyrene	Polystyrene	Polystyrene
Angle		90°	
dn/dc		0.185 g/ml	

The above characterisation data has been measured according to our Quality Control procedures.
Certificate of Analysis valid until expiry date – 11th January 2031
Agilent Manufacturing Site: Essex Road, Church Stretton, Shropshire, SY6 6AX, UK

G.K.Harmer P.C.Link

Quality Department

Issue 1 21st January 2021 COA STANDARDS 1 Rev 1.04