

Chem Service




Certificate of Analysis
Agilent Part No. 8500-2269 Lot# 311-113B
Performance Evaluation Sample for GC/MS Systems

Kit Contains 5 ampoules- 5x1 ml of the Following:

- 400ppm of Tris(1H,1H,5H-Octafluoropentyl)phosphate in Isooctane

Temperature Program 100°C(1 min) -> 200°C@ 10°C/min
Inlet Temperature 250°C
Transfer Temperature 280°C
Sample Size 1.0 ul
Column VF-5MS (30m x 0.25 mm x 0.25 um)
Flow 1.0 ml/min
Split Ratio 20:1

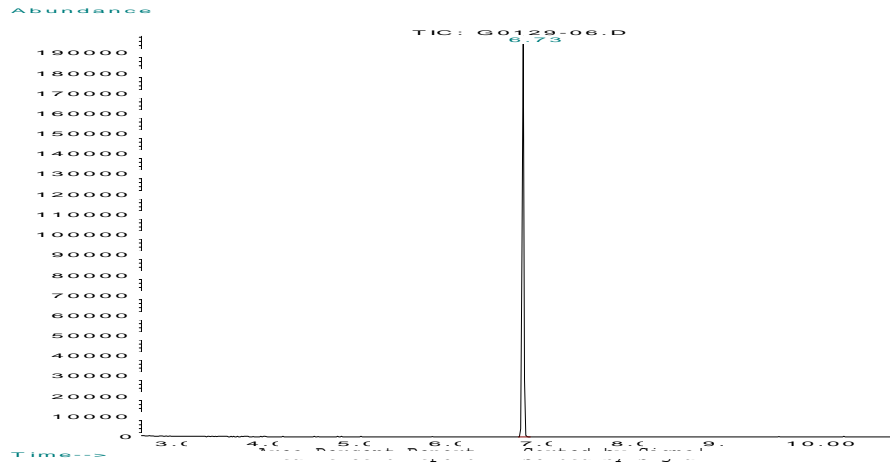

Information from Data File:
File : A:\G0129-06.D
Operator : mb
Acquired : 29 Jan 04 1:02 pm using AcqMethod METH2
Sample Name: Sp-8500-2269Z
Misc Info :
Vial Number: 76
CurrentMeth: C:\HPCHEM\MS\3\METHODS\METH2.M

| Retention Time | Area | Area % | Ratio % |
|------------------------|---------|---------|---------|
| Total Ion Chromatogram | | | |
| 6.731 | 2753621 | 100.000 | 100.000 |

Date of release: 1 January, 2004
Date of expiration: 1 January, 2007

John Conrad
John Conrad
CSM/TC