



Agilent Technologies



Certificate of Analysis

Agilent Part Number: 8500-8510

Sample Lot Number: LB78419

QC Number: Q174-105

QC Date: 23 JULY 2010

Concentration and Purity/Grade:

Neat Material

Fluoroether E-3 (CAS No.: 3330-16-3)



Gravimetric Conc.

Neat

Grade and/or Purity


GC MS 97.0%

Traceability:

This standard has been manufactured using ISO9001 quality procedures. High resolution gas chromatography mass spectroscopy was used to determine purity and verify the standard identity.

Analytical Spectrum or Chromatogram: EI Fragmentation Pattern

Abundance

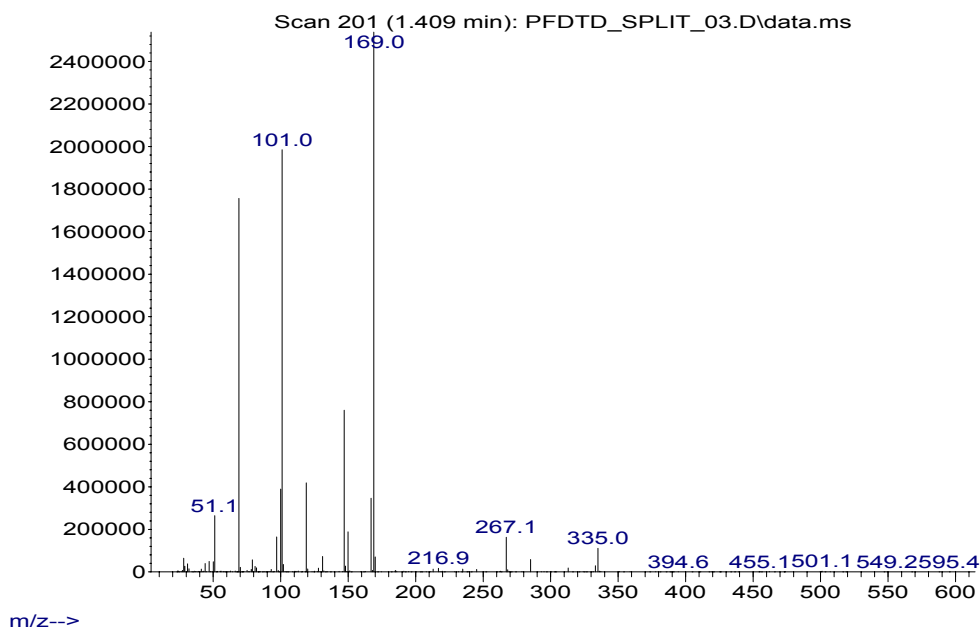

Comments:

No detectable contamination ions present from mass range 20-600 amu.

Date of Manufacture: 13 August 2010

Date of Expiration: 13 August 2015

Elwood Doughty
QA Manager
Supelco, Inc.