Agilent Technologies
Innovating the HP Way

PRAXAIR

Certificate of Analysis

Universal Gas Calibration Standard

Agilent Part Nos: 5183-4800, 5184-3541 **Sample Lot No:** 082501B

Concentrations:

Helium	0.101% (±5%)	n-Hexane	0.0501% (±10%)
Neon	0.0509% (±10%)	n-Heptane	0.0475% (±10%)
Hydrogen	0.102% (±5%)	Water content (H_2O)	<5 ppm
Oxygen	0.0512% (±10%)	Other impurities (HC's)	<1 ppm
Nitrogen	0.105% (±5%)		
Methane	Balance		
Ethane	0.0522% (±10%)		
Ethylene	0.0488% (±10%)		
Carbon Dioxide	0.0509% (±10%)		
Carbon Monoxide	0.0989% (±5%)		
Acetylene	0.0472% (±10%)		
Propane	0.0497% (±10%)		
Methyl Acetylene	0.0503% (±10%)		
n-Butane	0.0497% (±10%)		

Traceability:


This standard was produced gravimetrically using vendor quality procedures. Balances used are calibrated regularly, traceable to NIST. Standard concentrations were verified on an Agilent model 6890 gas chromatograph, using a Wasson valve switch, Variable Pressure Control and multiple packed/capillary columns.

Standards Used:

Praxair UGS Primary Standards, serial #s: H177474, 167228, 529117, 12064AW; source #SA4592

Analytical GC Chromatograms:

Analytical columns: MoleSieve 13X, HaySep DB, thick-film DB-1
TCD: 1.0 ml loop; He carrier at 35 ml/min; oven temp = 90degC
FID: 0.1 ml loop; He carrier at 30 ml/min; split ratio=25:1; Ramp 75degC for 6 min to 180degC for 3.75 min at 20degC/min

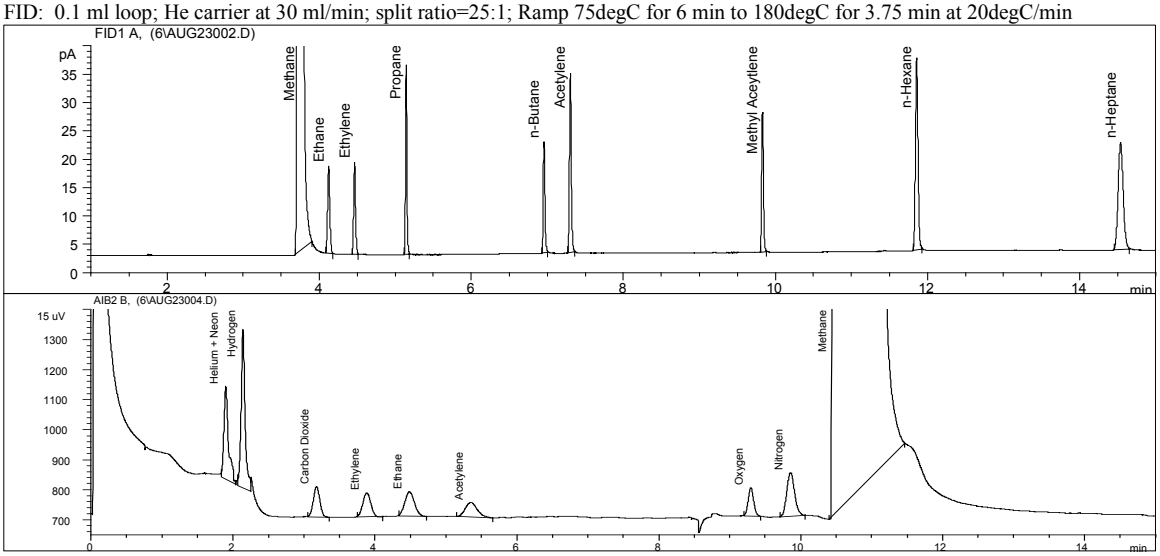

Date of Release: 25 August, 2001
Expiration Date: 25 August, 2003

Analyst: Alan M. Toth
Alan M. Toth, Chemist, Praxair, Inc.