

Certificate of Analysis

ESI Tuning Mix 100ml

Agilent Part Number: G2421A/G2421-60001 Sample Lot Number: A199600

Concentration (weight to volume) and Purity/Grades:

Neat Material	Gravimetric Conc.	Neat material Purity and/or Grade
Betaine (CAS NO.: 107-43-7)	< 0.01%	99.9%
Trifluoroacetic Acid Ammonium Salt (CAS NO.: 3336-58-1)	< 0.01%	99.8%
Hexamethoxyphosphazene (CAS NO.: 957-13-1)	< 0.01%	99.0%
Hexakis(2,2-Difluoroethoxy)Phosphazene (CAS NO.: 186817-57-2)	< 0.01%	99.0%
Hexakis(1H, 1H, 3H-Tetrafluoropropoxy)Phosphazene (CAS NO.: 58943-98-9)	< 0.01%	97.0%
Hexakis(1H, 1H, 5H-Octafluoropentoxy)Phosphazene (CAS NO.: 16059-16-8)	< 0.01%	98.0%
Hexakis(1H, 1H, 7H-Dodecafluoroheptoxy)Phosphazene (CAS NO.: 3830-74-8)	< 0.01%	97.0%
Hexakis(1H, 1H, 9H-Perfluorononyloxy)Phosphazene (CAS NO.: 186043-67-4)	< 0.01%	98.0%
Tris (heptafluoropropyl)-S-Triazine (CAS NO.: 915-76-4)	< 0.01%	99.1%


Solvent Composition:

Acetonitrile (CAS NO.: 75-05-8)	95.0%	HPLC grade 99.9%
DI Water (CAS NO.: 7732-18-5)	5.0%	De-ionized

Traceability:

This standard has been produced gravimetrically using ISO9001 quality procedures. . NIST traceable weights are used to verify balance calibration with the preparation of each lot. Concentration of analyte in solution is ug/ml +/- 0.5%, uncertainty based upon balance and Class A volumetric glassware. High-performance liquid chromatography mass spectroscopy was used to evaluate system performance.

Analytical Spectrum or Chromatogram: Fragmentation Pattern

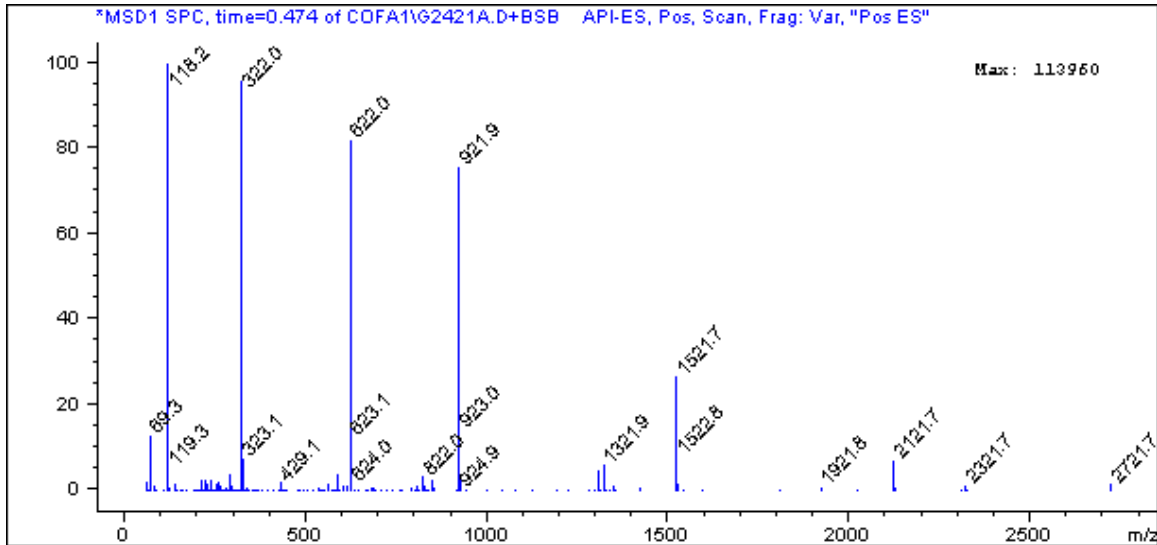

Agilent 1100 Series LC system:

G1354A Quaternary Pump (includes degasser)

G1313A Automatic liquid Sampler (ALS)

Agilent 1100 Series LC/MSD:

G1946D LC/MSD SL

G1948A API-Electrospray source

G1947A APCI source

G2421A Electrospray Tuning Calibrant

Column: None

Column Temp: N/A

Flow Rate: 0.4ml/min

Mobile Phase: 75:25 Acetonitrile/Water

Ionization Mode: Positive Electrospray

Nebulizer Pressure: 40 psi

Drying Gas Flow: 10L/min

Drying Gas Temp: 350 deg C

Scan Range: 50-3000


Step Size: 0.15amu

PRINCIPLE IONS

MASS	POS	NEG
1	118.09	112.99
2	322.05	431.98
3	622.03	601.98
4	922.01	1033.99
5	1521.97	1633.95
6	2121.93	2233.91
7	2721.89	2833.87

Date of Manufacture: 3 APRIL 2013

Date of Expiration: 3 APRIL 2015



Duane Funk
Quality Manager
Supelco, Inc