Agilent Technologies

SUPELCO

Certificate of Analysis

ES/APCI Positive Ion Performance

Agilent Part Number: G2423A Sample Lot Number: A301571

Purity: Reserpine NEAT – 99.0 +/- 0.2% (Weight percent)


Concentration: weight to volume	**Gravimetric Concentration**	**Purity**
Reserpine (CAS NO: 50-55-5)	0.005 mg/ml (+/- 0.05%)	99.0%

Solvent composition:

DI Water (CAS NO: 7732-18-5)	50%	(+/ -0.05%)	De-ionized
2-Propanol (CAS NO: 67-63-0)	50%	(+/- 0.05%)	Reagent Grade 99.6%

Traceability:
This standard has been produced gravimetrically using ISO9001 quality procedures. Balances used are calibrated regularly and meet the requirements of ISO. High-performance liquid chromatography mass spectroscopy was used to evaluate system performance.

Analytical Spectrum:

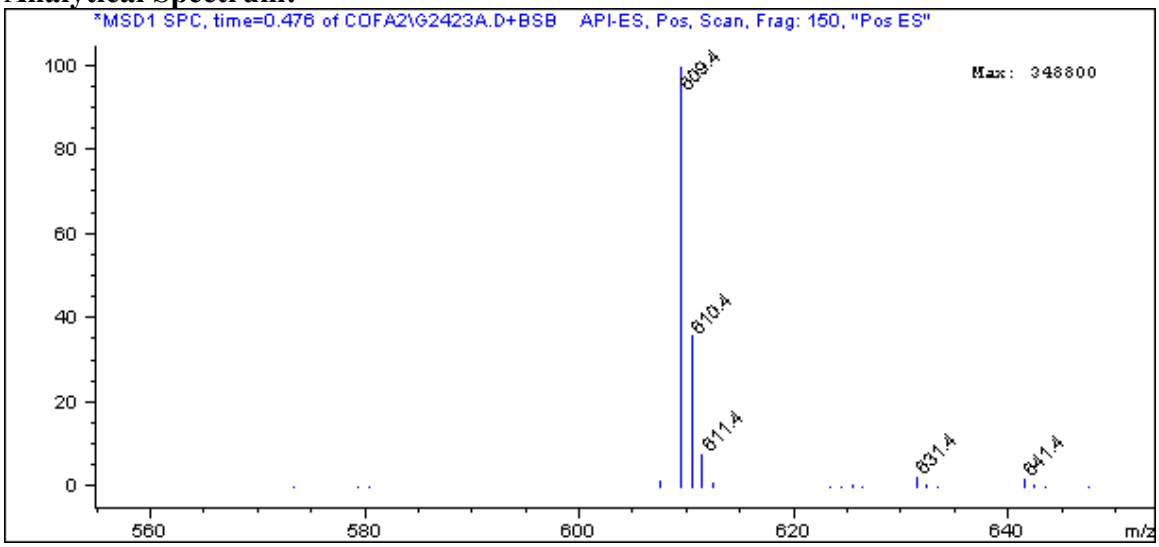

Manufacture Date: 10-December-2001
Expiration Date: 10-December-2003

Elwood Doughty
QA Manager
Supelco, Inc.