Agilent Technologies

SUPELCO

Certificate of Analysis

ES/APCI Positive Ion Performance

Agilent Part Number: G2423A Sample Lot Number: A398997


Purity: Reserpine NEAT – 99.0 +/- 0.2% (Weight percent)

Concentration: weight to volume
Reserpine (CAS NO: 50-55-5) less than 0.001% (+/-5%)

Solvent composition:
DI Water (CAS NO: 7732-18-5) 50% (+/-5%)
2-Propanol (CAS NO: 67-63-0) 50% (+/- 5%)

Traceability:
This standard has been produced gravimetrically using ISO9001 quality procedures. Balances used are calibrated regularly and meet the requirements of ISO. High-performance liquid chromatography mass spectroscopy was used to evaluate system performance.

Analytical Spectrum:

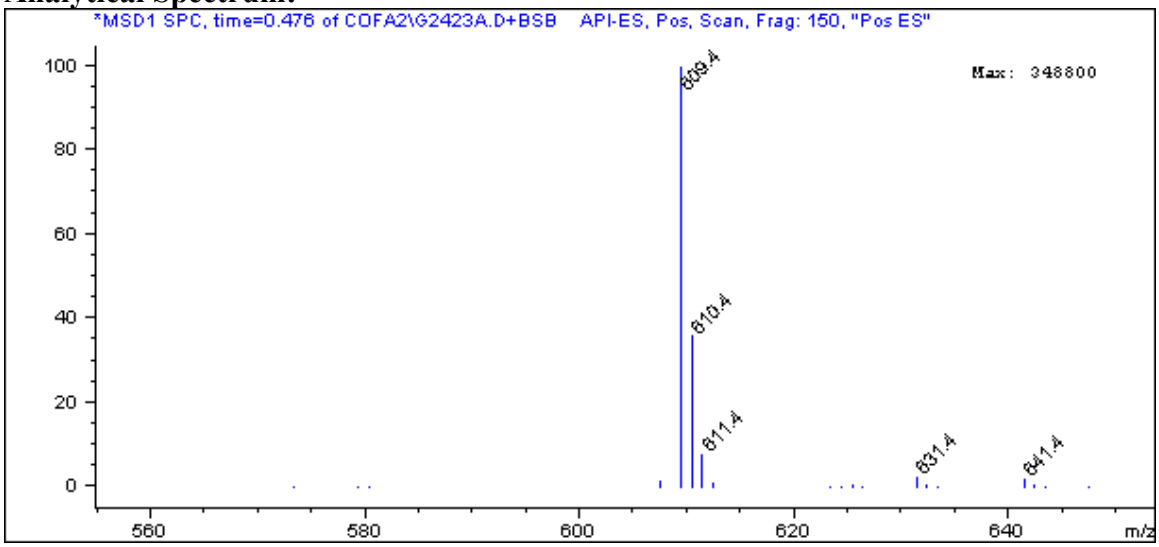

Manufacture Date: 16-JULY-2001
Expiration Date: 16-JULY-2003

Elwood Doughty
QA Manager
Supelco, Inc.