

Certificate of Analysis



Agilent Technologies, Inc. acquired Polymer Standards Service GmbH (PSS) on August 01st, 2022.

The Quality Certificate / Certificate of Analysis generated by PSS attached to this Letter is valid for the Product stated in the Certificate sold to You by Agilent Technologies, Inc or its subsidiaries.


Patrick Kunzweiler

Quality Manager
Liquid Phase Separation Division

Certificate of Analysis

Polymer type: Poly(acrylic acid) sodium salt
 Part No: PSS-PAA1.3M
 Lot No: PAA170114-2

Molar Mass Distribution

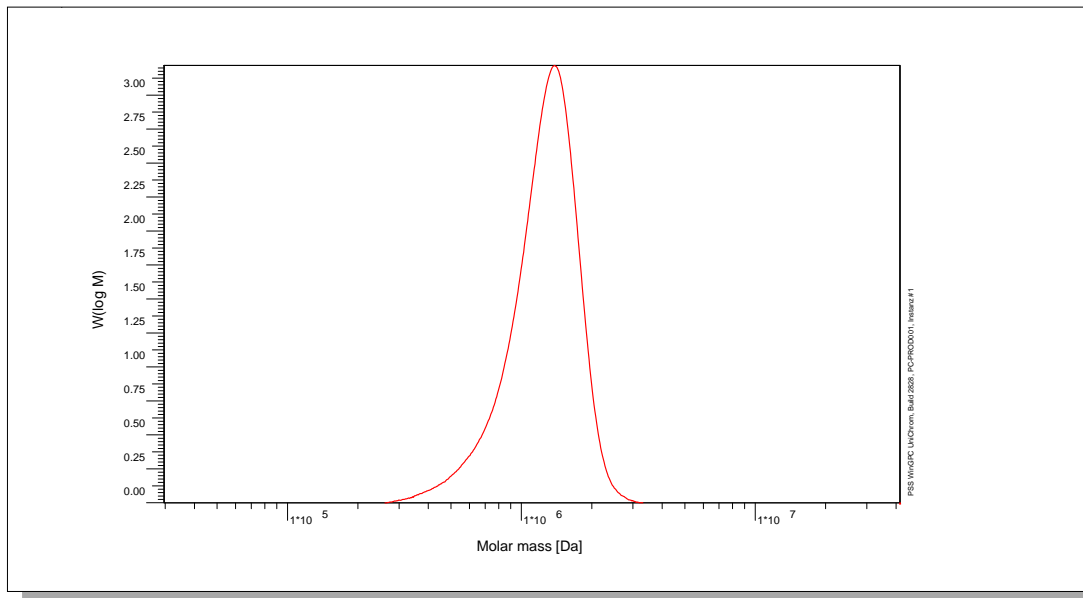

GPC/SEC - Conditions

Sample concentration	0,50 g/l	Inject volume	50 µl
Solvent	Water, 0.067M Na ₂ HPO ₄	Flow rate	1,00 ml/min
Precolumn [8 x 50 mm]	PSS SUPREMA 10µm	Temperature	30 °C
Columns [analytical, each 8 x 300 mm]	PSS SUPREMA 10µm 100Å / 3000Å / 3000Å	Operator	J.Preis
Data Acquisition Software	PSS WinGPC		

GPC/SEC - Results

Detector	Mw [Da]	Mn [Da]	Mp [Da]	PDI [mw/Mn]
PSS SECcurity RI	1300000	1160000	1390000	1,12

Note:


Mw = Weight average molecular weight
 Mn = Number average molecular weight
 Mp = Molar mass at the peak maximum
 PDI = Polydispersity Index

Storage: Store the tightly recapped polymer standard in a dry, dark, cool area; e.g. a refrigerator (4 °C).

Date of expiry: 2028/02/29 (See also product label)

Date of approval: 2023/02/24

Manufacture control according to PSS method of analysis


 Dr. J. Preis
 production manager

