



Certificate of Analysis

OFN EI Checkout Standard 1 pg/ μ L

**Agilent Part
Number:** 5188-5348

**Sample Lot
Number:** CM-5226

This analytical reference material was manufactured and verified in accordance with an ISO 9001 registered quality system, and the analyte concentrations were verified by an ISO 17025 accredited laboratory. The certified value for each analyte was determined gravimetrically.

Concentration:
octafluoronaphthalene 1.00 \pm 0.01 pg/ μ L (corrected for purity)


Solvent: isooctane

Calibrated Class A glassware and clean bottles were used in the manufacture of this standard. Balances used in the manufacture of this standard are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z-540-1 and ISO 9001.

Purities:
octafluoronaphthalene 99%
isooctane 99%

Typical Analytical Spectrum or Chromatography

Total ion chromatography under Agilent EI checkout conditions

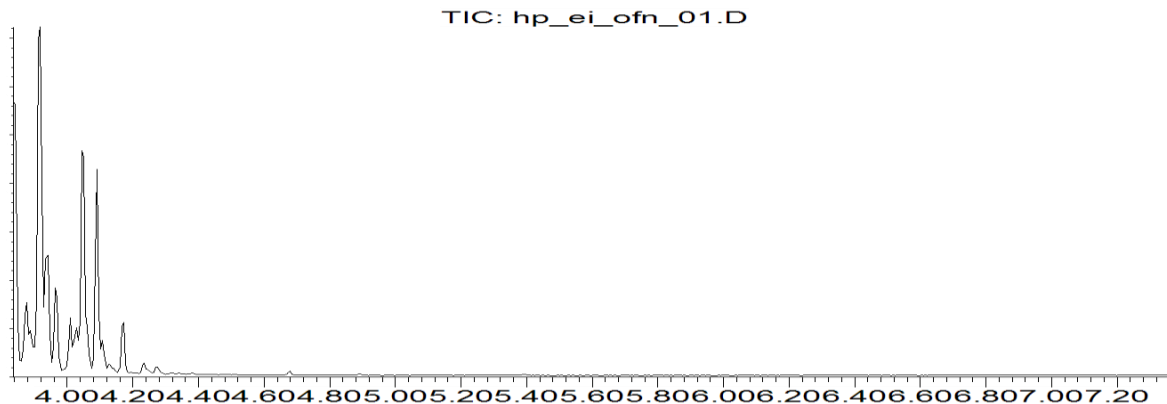

Date of release: 05 October 2015
Date of expiration: 31 October 2017


William J. Lea
Quality Assurance Manager