



Certificate of Analysis

Pesticide Analyzer Checkout Solution

**Agilent Part
Number:** 5190-0468

**Sample Lot
Number:** CR-5342A

This analytical reference material was manufactured and verified in accordance with an ISO 9001 registered quality system, and the analyte concentrations were verified by an ISO 17025 accredited laboratory. The certified value for each analyte was determined gravimetrically.

Analyte	CAS#	Analyte Lot	Purity %	Certified Value
dichlorvos	000062-73-7	RM10844	97.7	10.0 ± 0.1 µg/mL
mevinphos	007786-34-7	RM10675	98.3	10.0 ± 0.1 µg/mL
ethalfluralin	055283-68-6	RM11766	99.5	10.0 ± 0.1 µg/mL
trifluralin	001582-09-8	RM11013	99.5	10.0 ± 0.1 µg/mL
atrazine	001912-24-9	RM10318	98.7	10.0 ± 0.1 µg/mL
lindane	000058-89-9	RM02694	99.9	10.0 ± 0.1 µg/mL
chlorpyrifos-methyl	005598-13-0	RM09206	99.6	10.0 ± 0.1 µg/mL
heptachlor	000076-44-8	RM03111	99.9	10.0 ± 0.1 µg/mL
malathion	000121-75-5	RM12444	98.0	10.0 ± 0.1 µg/mL
chlorpyrifos	002921-88-2	RM09198	99.9	10.0 ± 0.1 µg/mL
dieltrin	000060-57-1	RM03957	98.0	10.0 ± 0.1 µg/mL
4,4'-DDE	000072-55-9	RM02892	99.9	10.0 ± 0.1 µg/mL
hexazinone	051235-04-2	RM03124	99.5	10.0 ± 0.1 µg/mL
propargite	002312-35-8	RM11752	99.3	10.0 ± 0.1 µg/mL
leptophos	021609-90-5	RM03755	98.3	10.0 ± 0.1 µg/mL
mirex	002385-85-5	RM00220	99.0	10.0 ± 0.1 µg/mL
fenarimol	060168-88-9	RM07334	99.9	10.0 ± 0.1 µg/mL
coumaphos	000056-72-4	RM12041	99.4	10.0 ± 0.1 µg/mL
ethofenprox	080844-07-1	RM09144	99.8	10.0 ± 0.1 µg/mL
deltamethrin	052918-63-5	RM10595	99.5	10.0 ± 0.1 µg/mL

Solvent: acetone

Calibrated Class A glassware and clean bottles were used in the manufacture of this standard. Balances used in the manufacture of this standard are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z-540-1 and ISO 9001.

Date of release: 12 April 2018


Date of expiration: 31 May 2019


John Russo
President


Monica Bourgeois
Director of QA/RA



Agilent Technologies

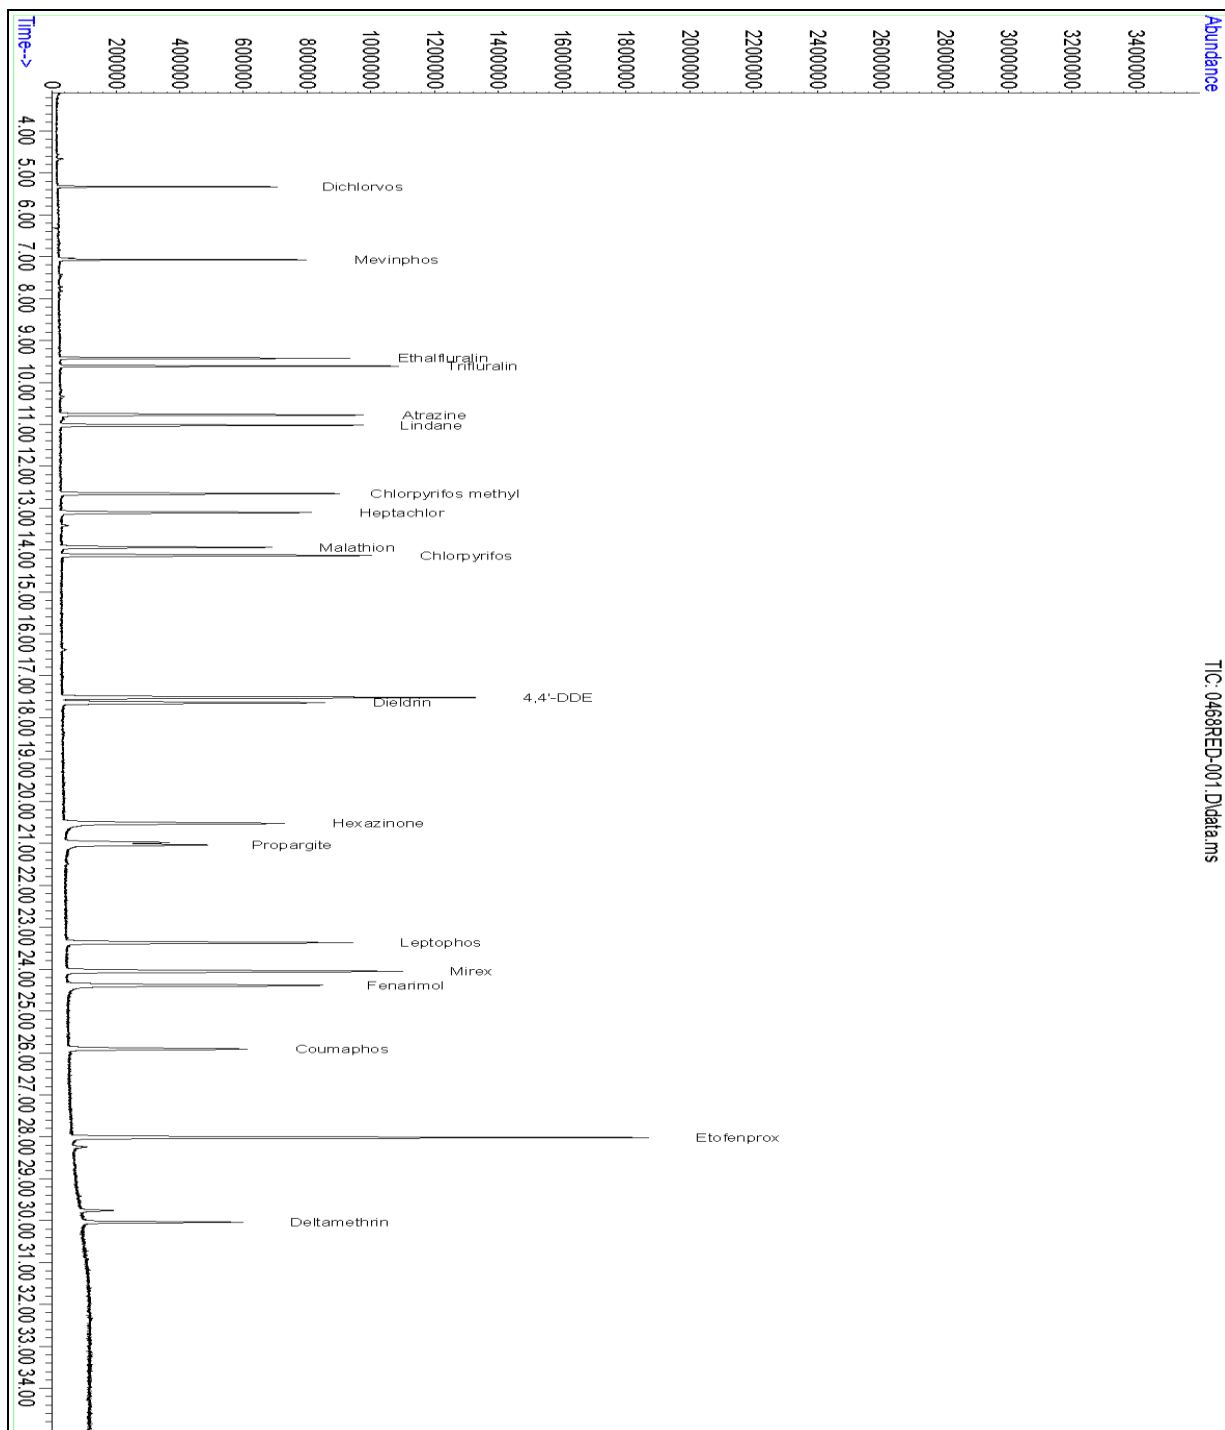

John Russo
President

Monica Bourgeois
Director of QA/RA