

Hydrocarbon C₁ to C₅s on HP-PLOT U Column

Column: HP-PLOT U

0.32 mm x 30 m I.D., 10 µm

P/N: 19091P-U04

Oven: 60°C for 7min


60-180°C at 10°C/min

Inlet: 180°C, Split ratio 30:1

Detector: FID 200°C

Sample: 5 µL HC

- | | | | |
|----|------------------|-----|--|
| 1. | C ₁ | 8. | Propyne |
| 2. | Ethylene | 9. | I-C ₄ |
| 3. | C ₂ s | 10. | C ₄ s |
| 4. | Acetylene | 11. | nC ₄ + cis-C ₄ = |
| 5. | C ₃ s | 12. | i-C ₄ = |
| 6. | Cyclopropane | 13. | t-C ₄ = |
| 7. | Propadiene | 14. | C ₅ s |

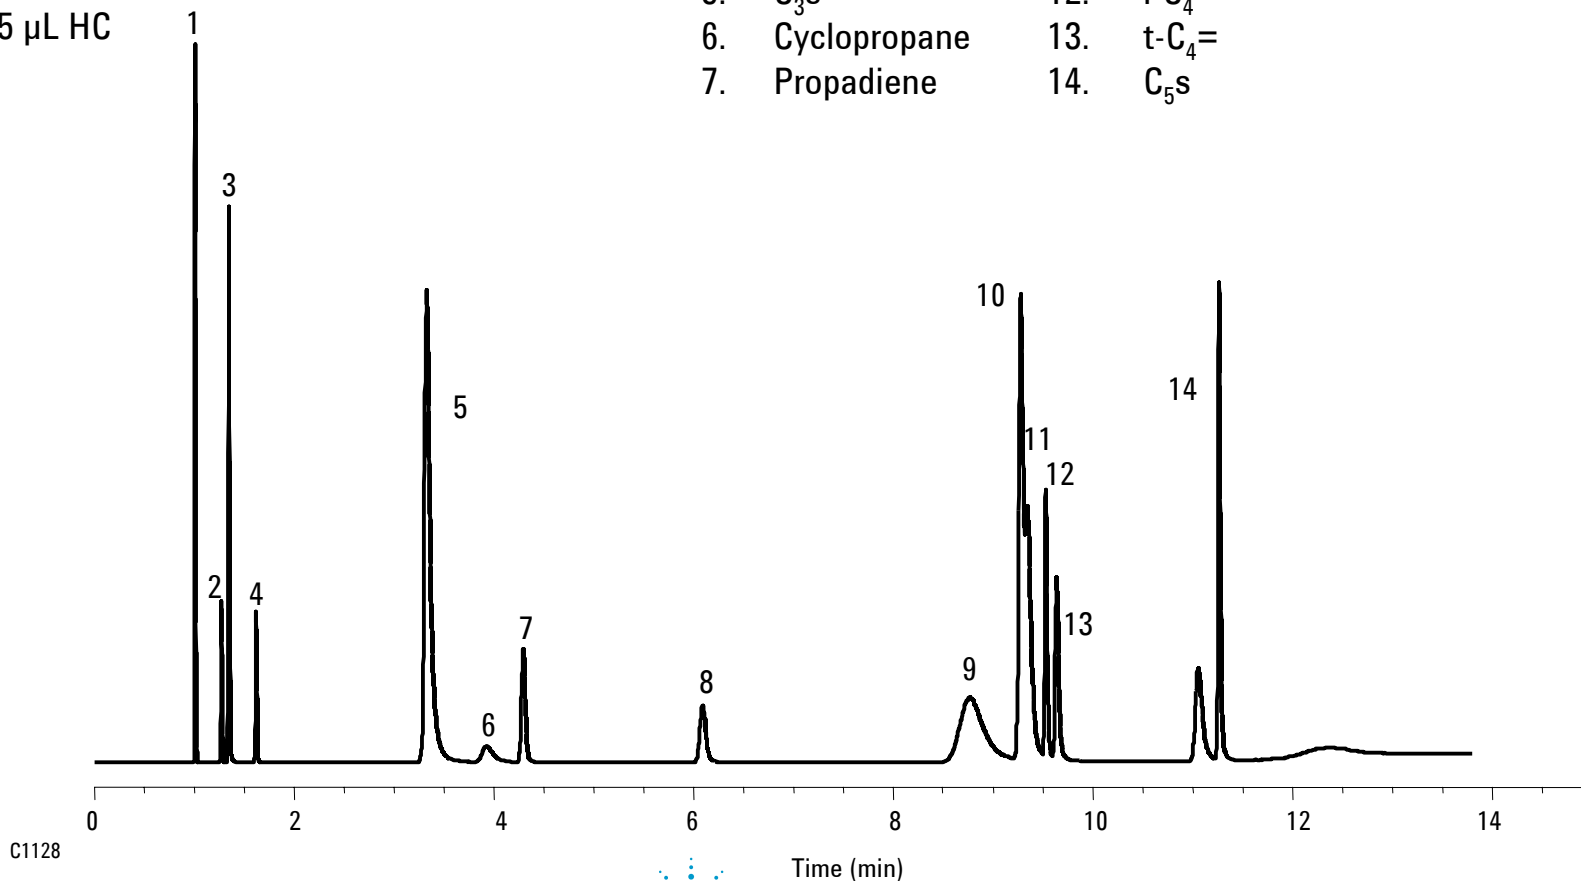

Agilent Technologies