


Volatile Solvents On HP-PLOT U Column

Column: HP-PLOT U
0.32 mm x 30 m I.D., 10 µm
P/N: 19091-U04
Oven: 150°C
Inlet: 180°C, split ratio 30:1
Detector: FID, 200°C
Sample: 1µL Liquid

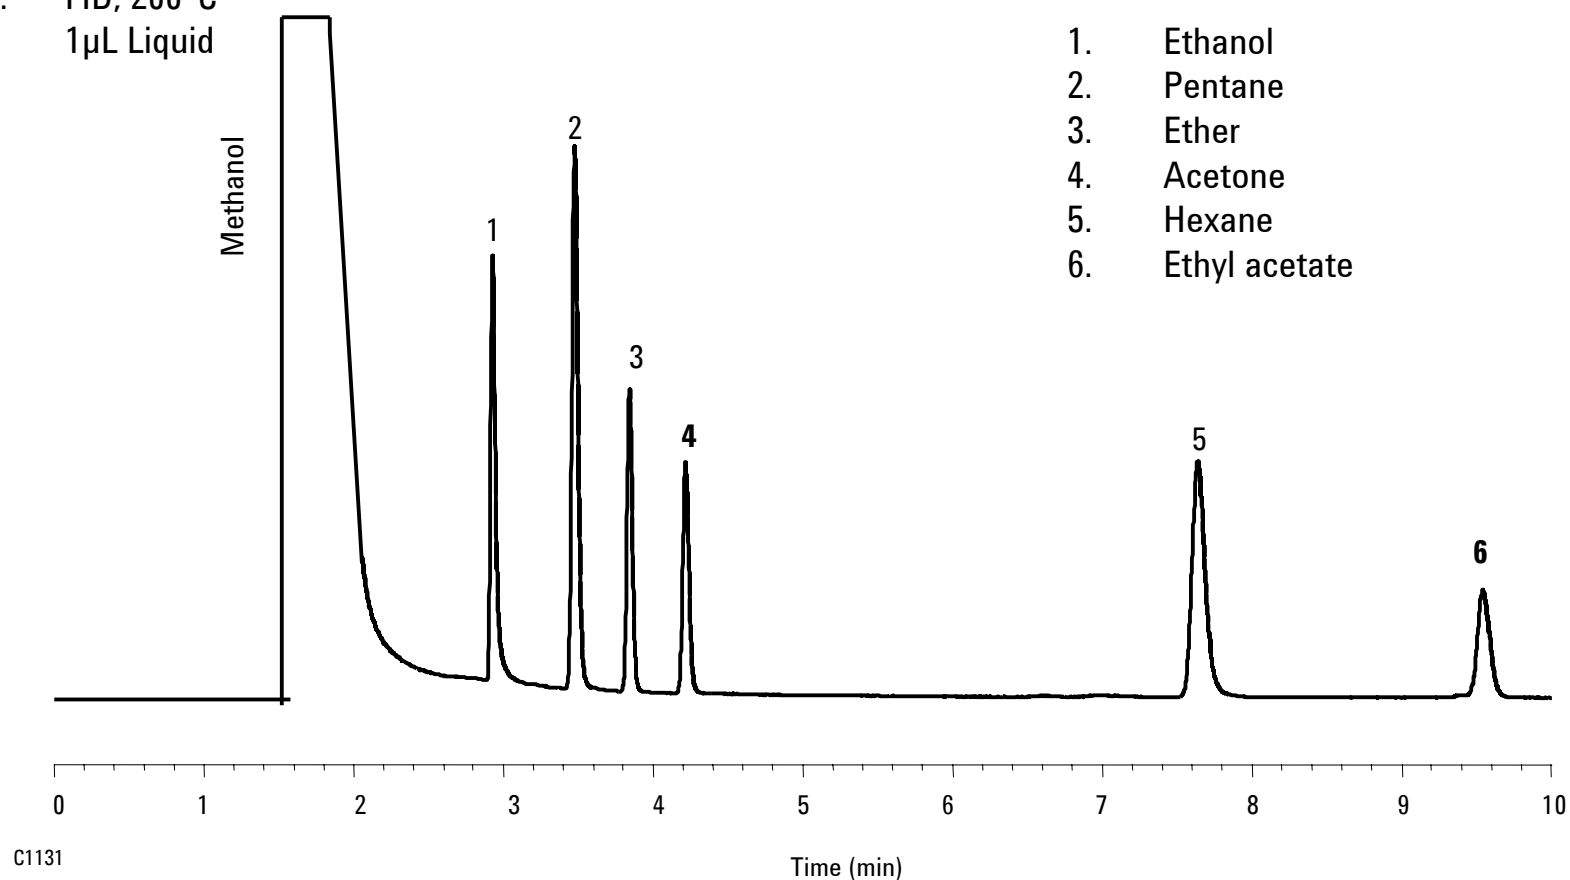

C1131