


# Acetone

**Column:** HP-PLOT U  
0.53 mm x 30 m I.D., 40  $\mu$ m  
**P/N:** 19091P-U04  
**Oven:** 150°C for 1 min  
150-190°C at 10°C/min  
190°C for 4 min  
**Inlet:** 150°C, split ratio 50:1  
**Detector:** TCD  
**Sample:** 10  $\mu$ L acetone, HPLC grade

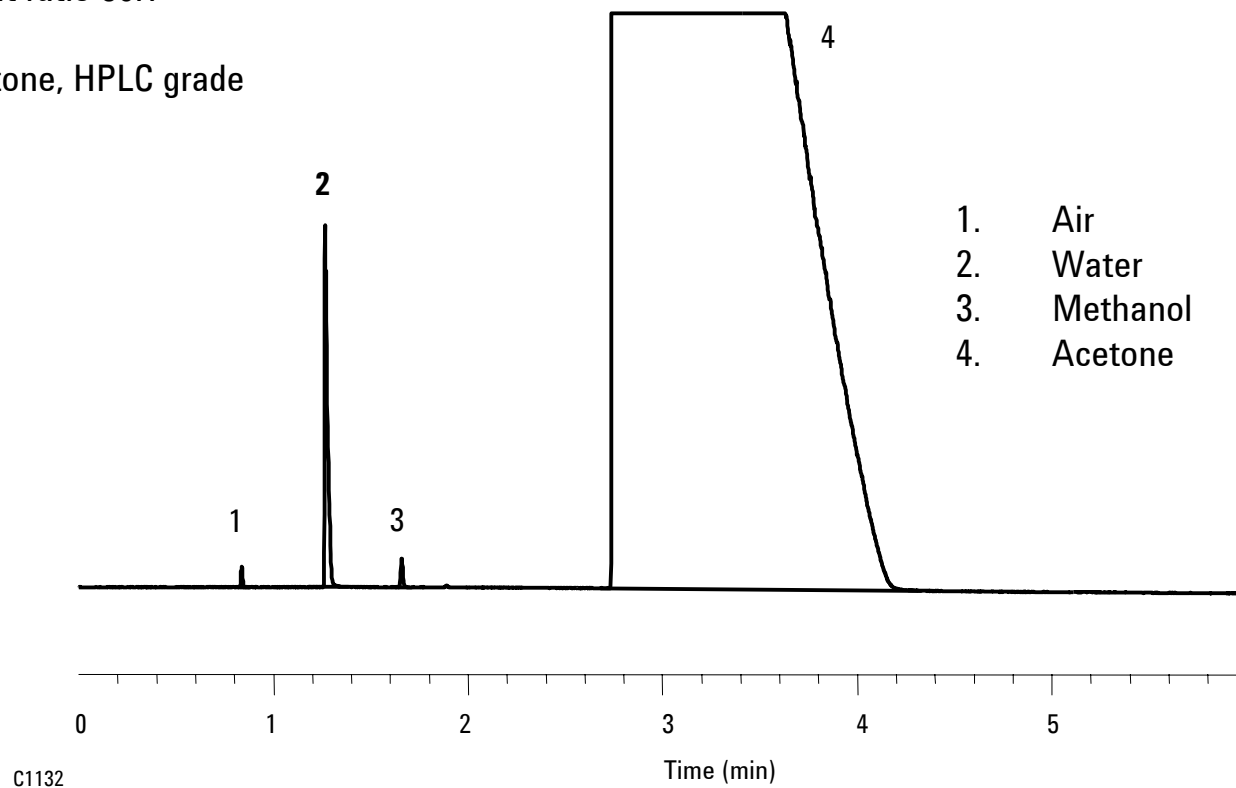

**Agilent Technologies**