

Ethyl Acetate on HP-PLOT U Column

Column: HP-PLOT U
0.32 mm x 30 m I.D., 10 µm

P/N: 19091P-U04

Oven: 100°C for 25 min
100-190°C at 10°C/min
190°C for 5 min


Carrier: Hydrogen, 1.5mL/min

Inlet: 180°C, Split ratio 30:1

Detector: FID, 200°C

Sample: 5 µL HPLC grade Et acetate

1. Methanol
2. Ethanol
3. Acetic Acid ?
4. Methyl acetate
5. Ethyl acetate

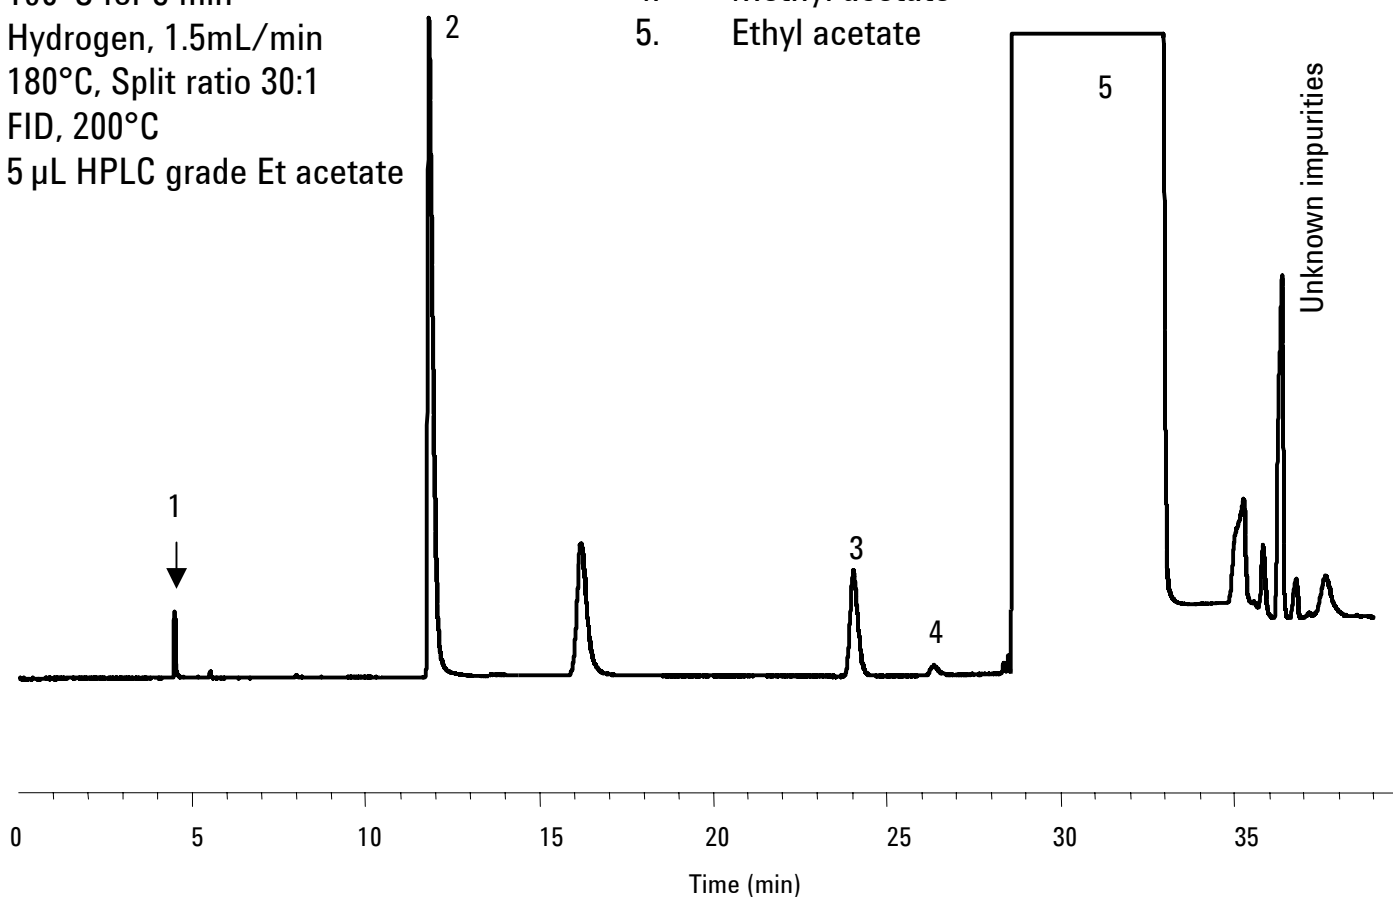

C1133