

Acetic acid on HP-PLOT U column

Column: HP-PLOT U
0.32 mm x 30 m I.D., 10 µm


P/N: 19091P-U04

Oven: 125°C for 1min
125-180°C at 10°C/min
180°C for 4 min

Inlet: 150°C, split ratio 50:1

Detector: TCD

1. Air
2. Water
3. Methanol
4. Formic acid
5. Acetic acid

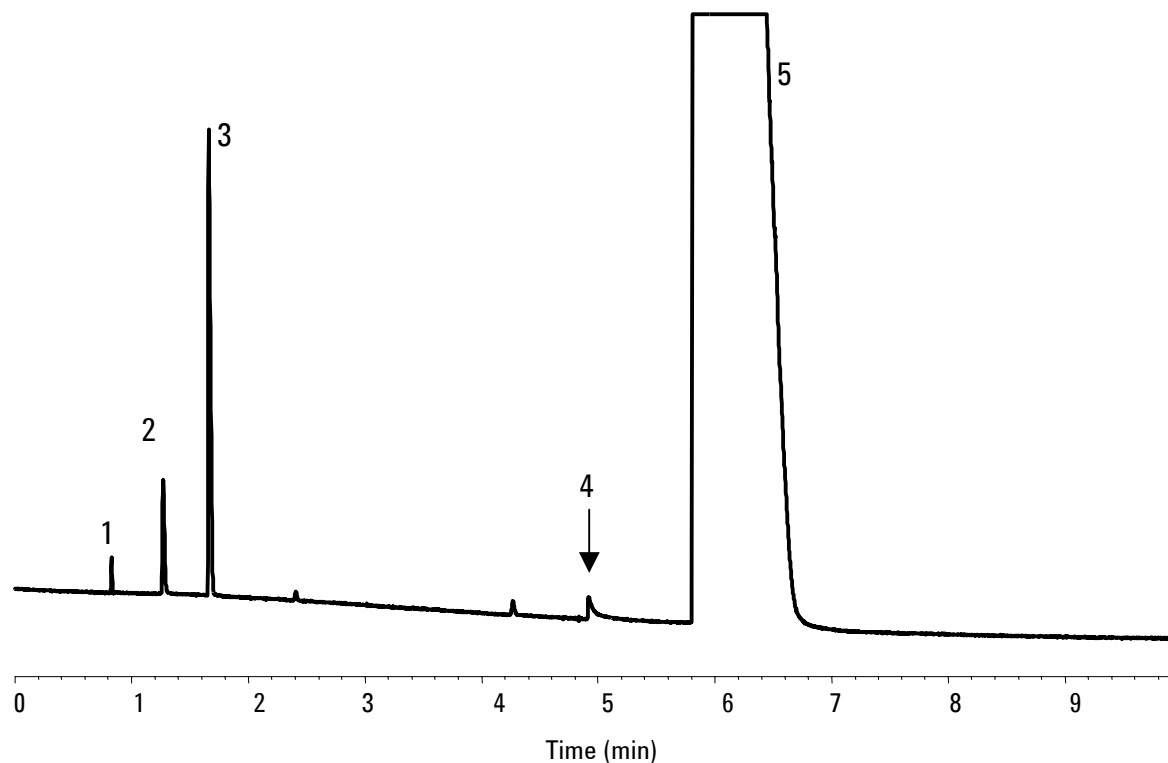

C1134



Agilent Technologies