

# Ethylene Oxide Gas on PLOT U Column

**Column:** HP-PLOT U  
0.32 mm x 30 m I.D., 10  $\mu$ m

**P/N:** 19091P-U04

**Oven:** 60°C for 5 min  
60-150°C at 10°C/min  
150°C for 2 min


**Carrier:** Hydrogen, 1.5 mL/min

**Inlet:** 180°C, Split ratio 30:1

**Detector:** FID, 200°C

**Sample:** 5  $\mu$ L

1. C<sub>1</sub>
2. C<sub>2</sub>
3. C<sub>3</sub>
4. Ethylene oxide + i-C<sub>4</sub>
5. C<sub>4</sub>
6. C<sub>5</sub>

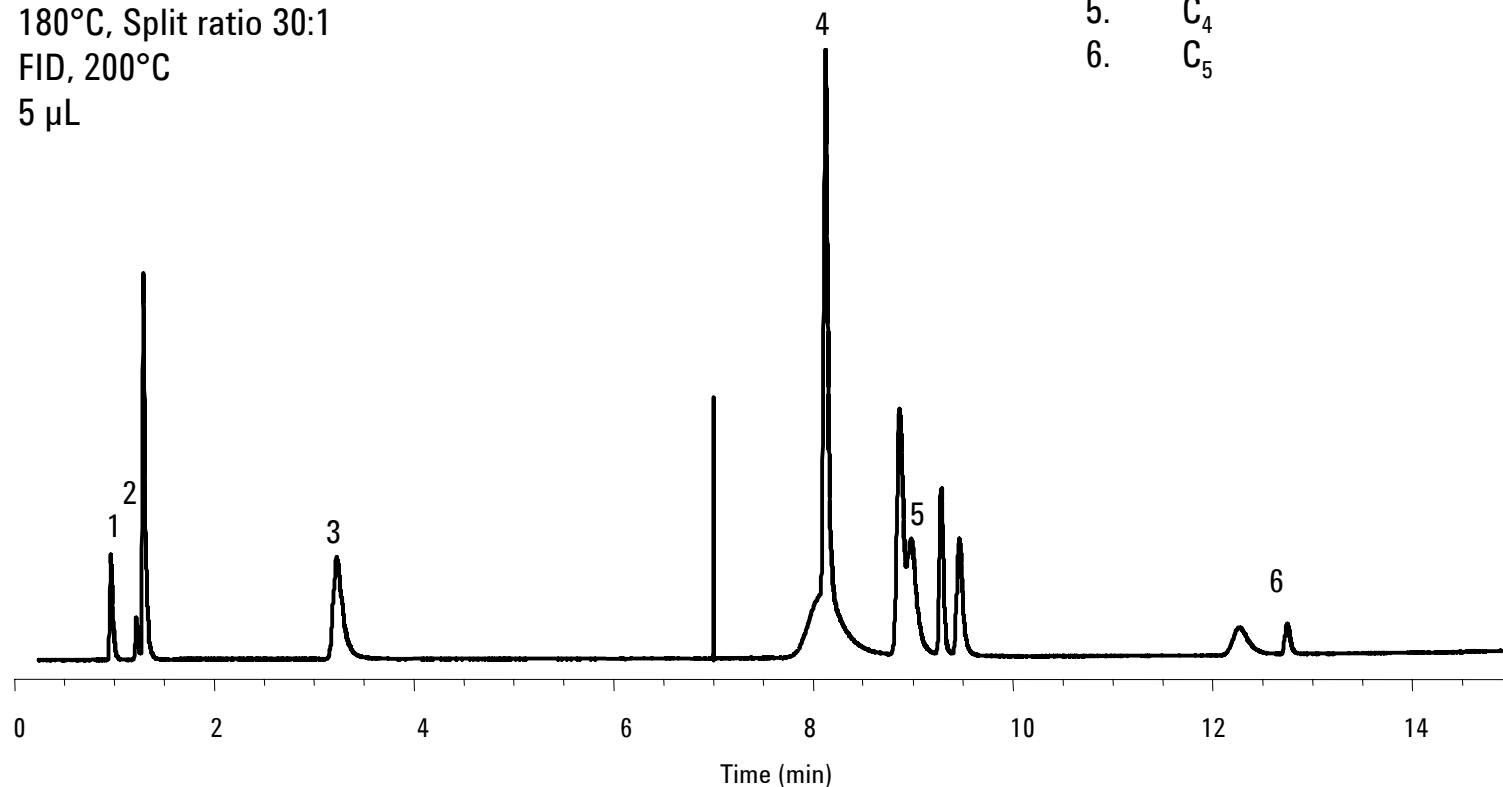

C1136