




Agilent ICP Go Software

Elemental analysis made easy

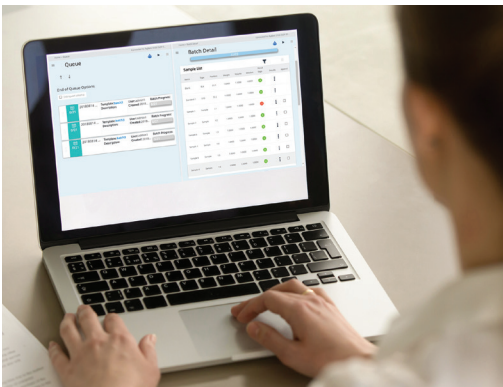


Go anywhere — ICP Go is browser-based, allowing remote monitoring of your analysis from any PC or tablet. One or more instruments can be monitored by using multiple browser tabs.

Focus on the essentials


ICP Go¹ is a simple, browser-based software interface that makes routine operation of your Agilent ICP-MS easier than ever. It is compatible with all Agilent 7700, 7800, and 7900 ICP-MS instruments and allows even new or occasional users to confidently run an analysis.

With ICP Go you can:


- Quickly set up and run sample batches from stored templates. This functionality provides a high level of control over batches and reduces the possibility of method errors that can cause inconsistent results and costly reruns.
- Control your entire analytical run, from igniting the plasma through to analyzing samples. You can easily queue urgent samples for immediate analysis, and monitor the instrument status remotely.
- New user training can be completed in less than a day. This reduces the costs of initial training, and makes it much easier for operators to transfer between analytical techniques. ICP Go's clear screen layout and simple workflow also supports the crosstraining of analysts, giving you more staffing flexibility. This means that your senior analysts can focus on more advanced tasks, such as optimizing lab efficiency.

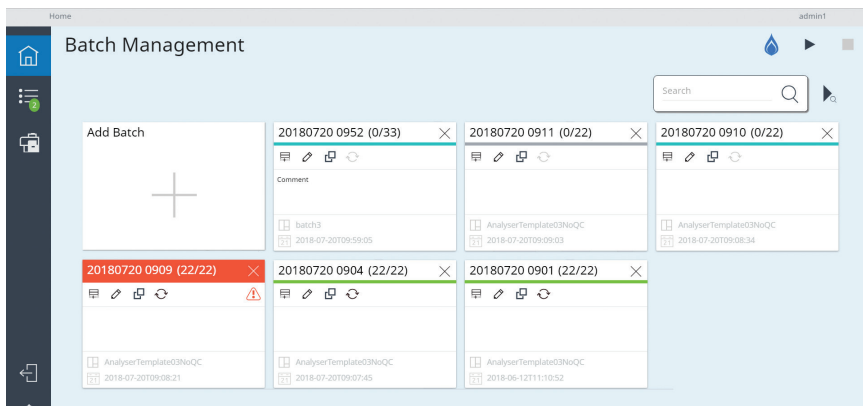

Step 1. Create a new batch of samples by selecting the method template and importing or entering the sample names.

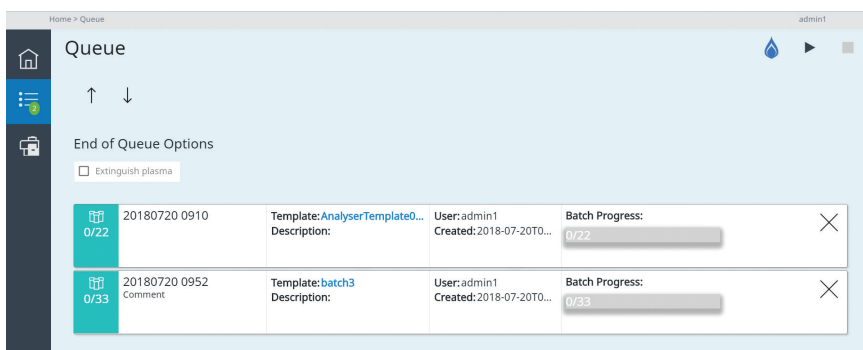

Step 2. Add the batch to the queue for analysis. The status of each batch in the queue is displayed onscreen.

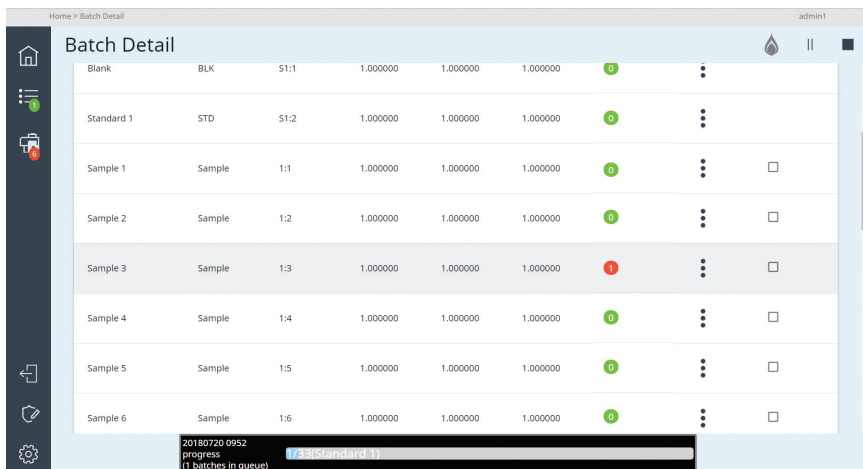

Step 3. Color-coded flags show the run status, allowing easy identification of errors, such as QC failures.

1. The Agilent ICP Go Software is currently available in North America and Western Europe only.

Learn more:

www.agilent.com/chem/icpms

This information is subject to change without notice.

© Agilent Technologies, Inc. 2018
Published in the USA, September 26, 2018
5994-0213EN

Analyze samples in 3 steps

After loading samples into the autosampler, analyzing them requires only three steps:

1. Create a new batch by importing or manually entering the sample names into your chosen method template.
2. Add the batch to the Queue. You can change the order of batches, if necessary. Analysis of queued batches starts automatically if the Queue is already running. Otherwise, click the Start icon to run the new batch.
3. You can monitor the status of the analysis using the color-coded flags, displayed during the run.

Compatibility

ICP Go is compatible with:

- Agilent 7700, 7800 and 7900 ICP-MS instruments
- ICP-MS MassHunter version 4.5 or later, running on Microsoft Windows 10 operating system, version 1703 or later
- Agilent ASX 520 autosampler
- Agilent SPS 4 autosampler

Ordering information

ICP Go is included with the Agilent ICP-MS Water Analyzer, or can be purchased separately, as an option for ICP-MS MassHunter.