


You Have 24 Hours in a Day. How Do You Want to Spend Them?

By simply using Agilent Captiva EMR—Lipid for sample preparation, you can minimize three major time consumers caused by lipid build-up, with better data accuracy and precision.

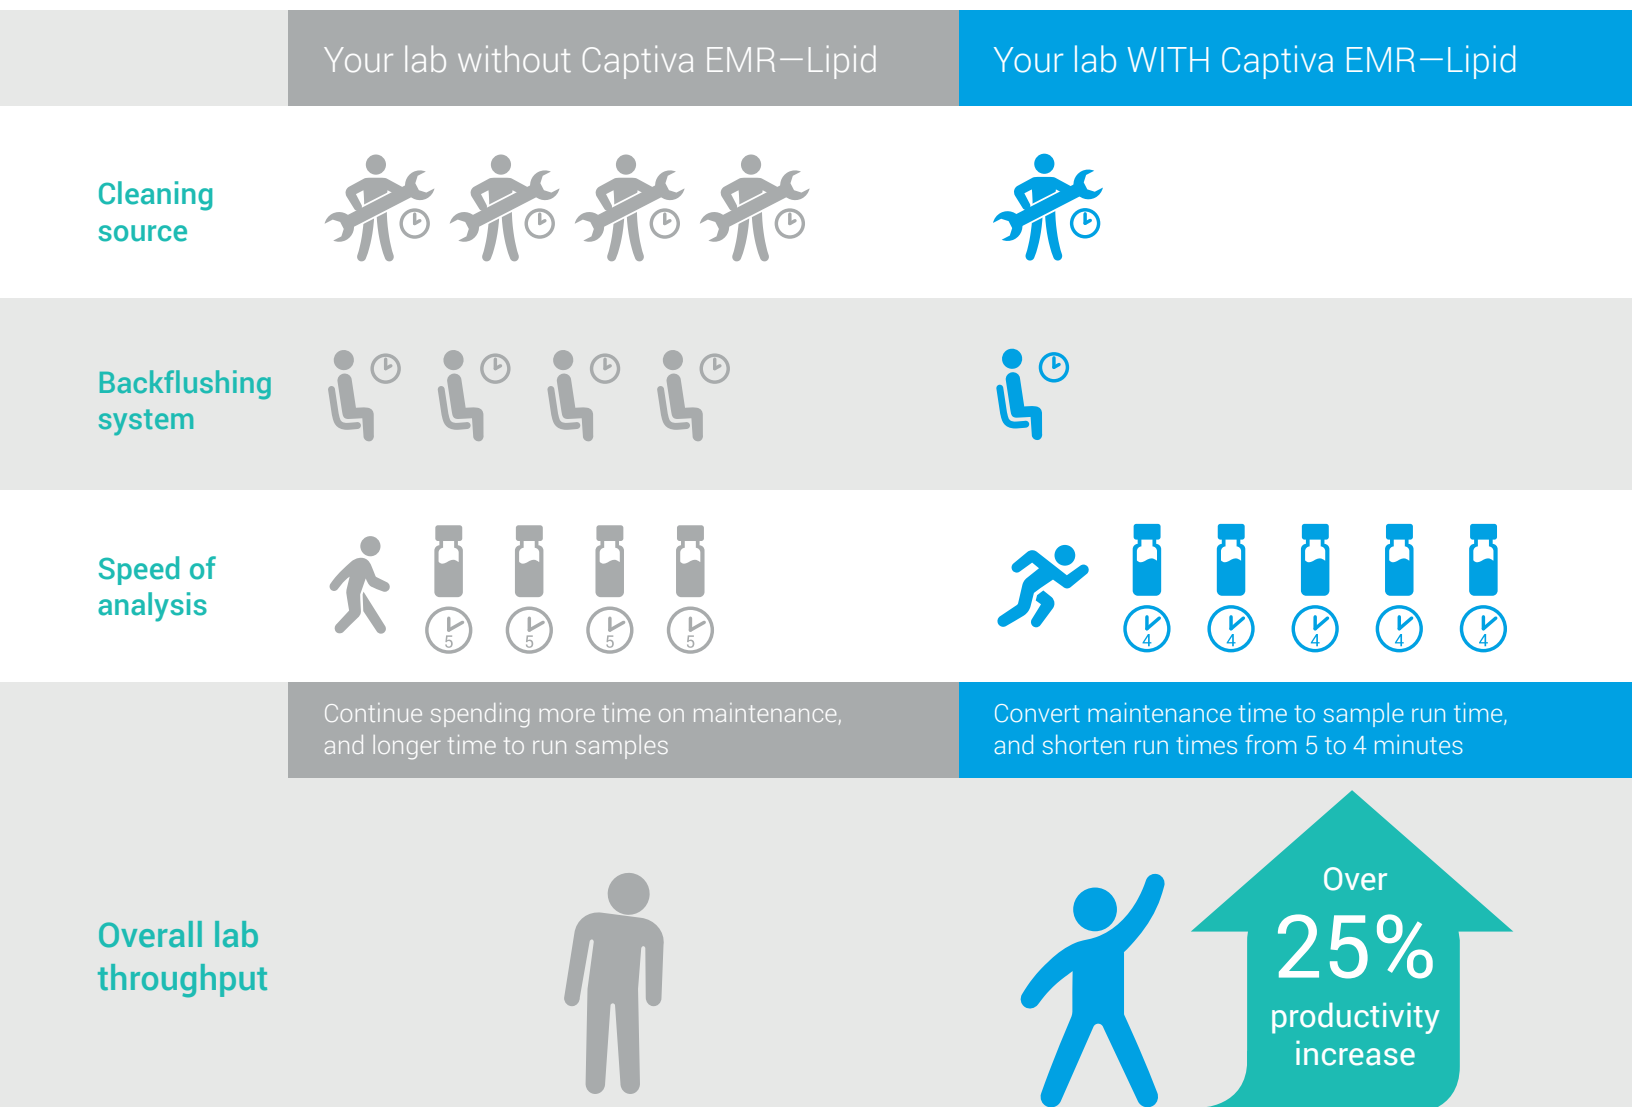

This scenario is based on a high-throughput lab running approximately 6500 samples per month on a single instrument (LC/MS/MS). This lab is striving to run 24/7 with a 5-minute LC run time. At this lab, technicians need to flush the column routinely and clean the MS source once a month in its current state.

This information is subject to change without notice.

© Agilent Technologies, Inc. 2018
 Published in the USA, July 25, 2018
 5994-0111EN

Interested in learning more about potential productivity improvements? Start exploring:
www.agilent.com/chem/did-you-know