


## Using the Agilent SPS 3 Autosampler with Cary Instruments

For your Agilent SPS 3 autosampler to operate with the Cary WinUV software, you need to set the DIP switch on the side panel of the autosampler to position 6. Refer to the below figure.



This information is subject to change without notice.

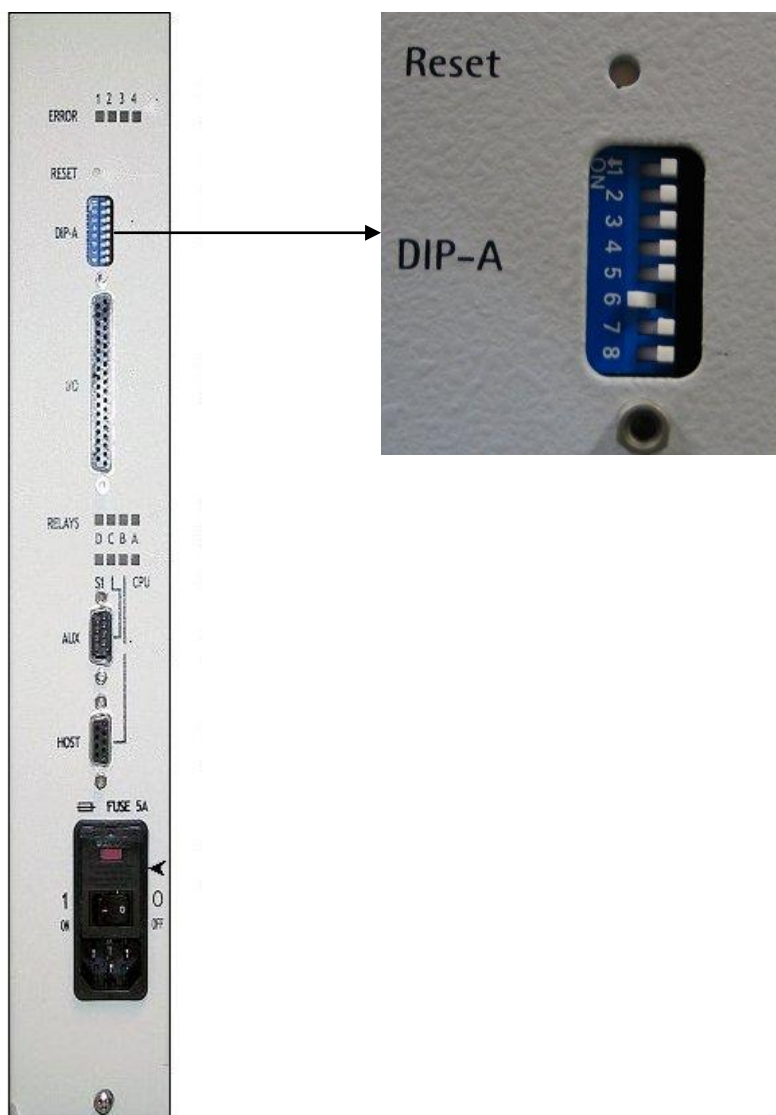

8510215000

Part Number: 8510215000

Edition 01/11

Issue 2

Printed in Australia

© Agilent Technologies, Inc. 2004, 2011

Agilent Technologies

679 Springvale Road

Mulgrave, VIC 3170