



Agilent InfinityLab Ultivo LC/TQ

Site Preparation Guide

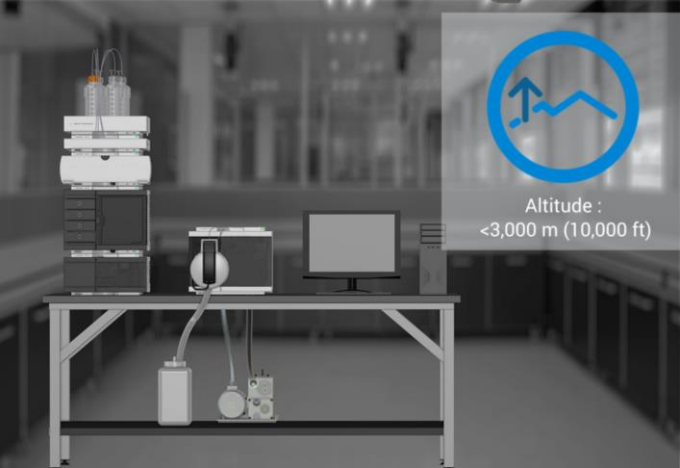

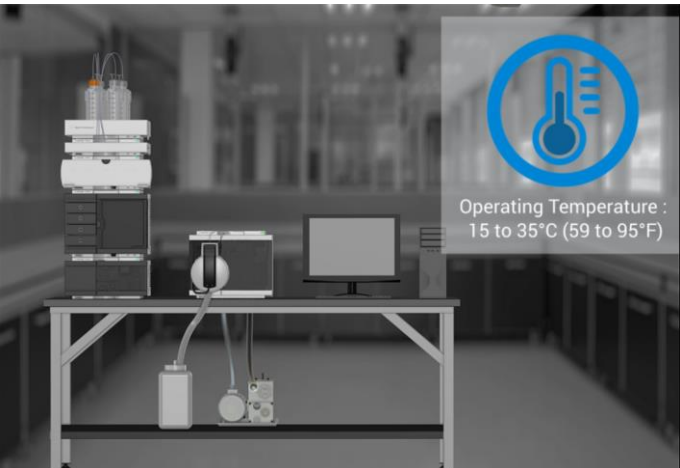


Operating environment

Environmental Conditions

The Ultivo LC/TQ is designed for use in the following environmental conditions for Class 1 Laboratory equipment, as specified by the International Electro-technical Commission (IEC).

Equipment class	Class 1 Laboratory equipment
Pollution	Degree 2
Installation	Category II
Environment	Indoor use
Altitude	Not to exceed 3000 m (10,000 ft)
Electrical supply	200 to 240 VAC, 50/60 Hz
Mains supply voltage	Fluctuations not to exceed 10% of nominal supply voltage
Operating temperature	15 to 35°C (59 to 95°F)
Humidity	< 85% RH at 35°C

1	Altitude: Not to exceed 3000 m (10,000 ft.)	 <p>Altitude : <3,000 m (10,000 ft)</p>
2	Electrical supply: 200 to 240 VAC 50/60 Hz Mains supply voltage: Fluctuations not to exceed 10% of nominal supply voltage.	 <p>Electrical Supply : 200 to 240 VAC, 50/60 Hz</p>
3	Operating Temperature: 15 to 35°C (59 to 95°F)	 <p>Operating Temperature : 15 to 35°C (59 to 95°F)</p>

4 Humidity: <85% RH at 35°C

