



Agilent InfinityLab LC/MSD iQ

Site Preparation Guide







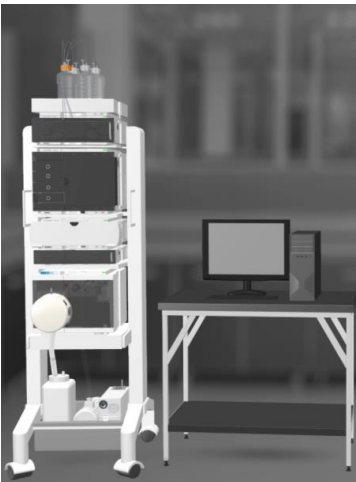

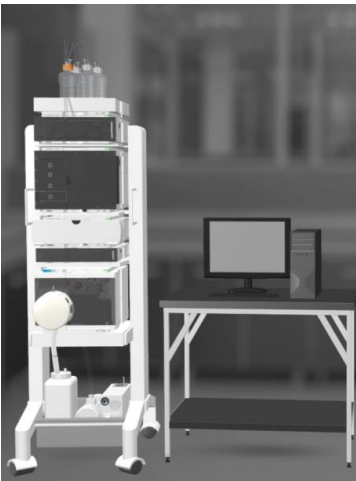

Operating environment

Environmental Conditions

The InfinityLab LC/MSD iQ is designed for use in the following environmental conditions for Class 1 Laboratory equipment, as specified by the International Electro-technical Commission (IEC).

Equipment class	Class 1 Laboratory equipment
Pollution	Degree 2
Installation	Category II
Environment	Indoor use
Altitude	Not to exceed 3000 m (10,000 ft)
Electrical supply	InfinityLab LC/MSD iQ: 120 VAC or 220 VAC
	MS40+ pump: 120 VAC with optional transformer, or 220 VAC
Mains supply voltage	Fluctuations not to exceed 10% of nominal supply voltage
Operating temperature	15 to 35°C (59 to 95°F)
Humidity	< 85% RH at 35°C

1	Altitude: Not to exceed 3000 m (10,000 ft.)	
2	InfinityLab LC/MSD iQ electrical supply : 120 or 220 VAC Mains supply voltage: Fluctuations not to exceed 10% of nominal supply voltage.	

3	MS40+ pump electrical supply:120 VAC (with optional transformer), or 220 VAC.	  <p>MS40+ Pump Electrical Supply: 120 VAC (with optional transformer), or 220 VAC</p>
4	Operating Temperature: 15 to 35°C (59 to 95°F)	  <p>Operating Temperature : 15 to 35°C (59 to 95°F)</p>
5	Humidity: <85% RH at 35°C	  <p>Humidity : < 85% RH at 35°C</p>