


Free Fatty Acids

Column: HP-5MS
30 m x 0.25 mm I.D., 0.5 μ m
P/N 19091S-133
Carrier: Hydrogen at 40 cm/sec
Oven: 100°C Isothermal
Injector: Split 50:1, 250°C
5 ng/on-column
Detector: FID, 300°C

1. Isovaleric acid
2. Hexanoic acid
3. 2-Ethylhexanoic acid

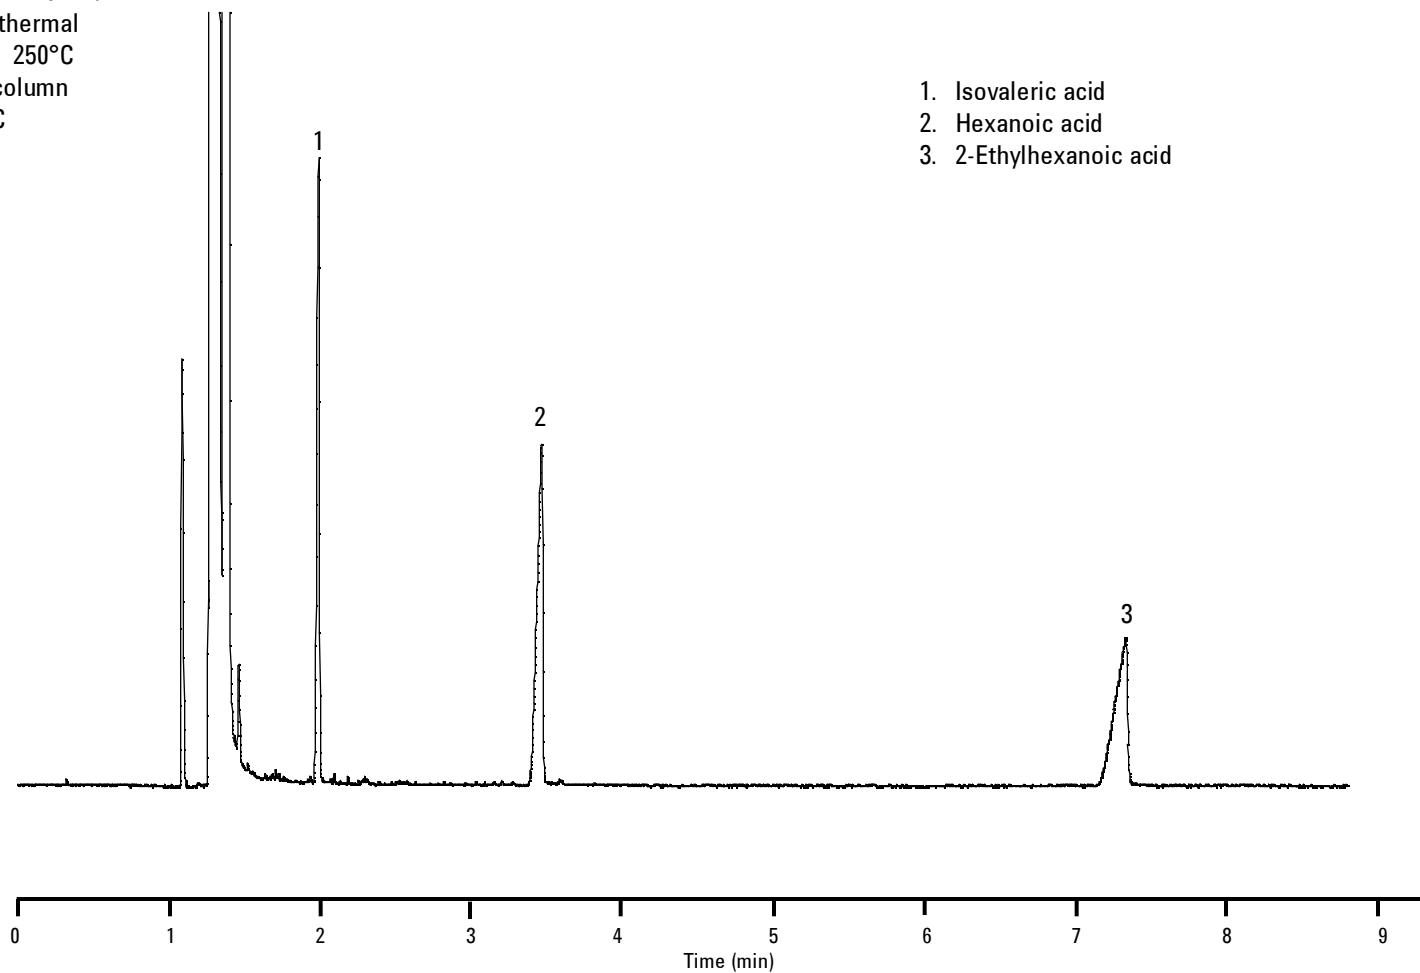

C1092